

**Fig. 1**

U.S. Patent & Trademark Office

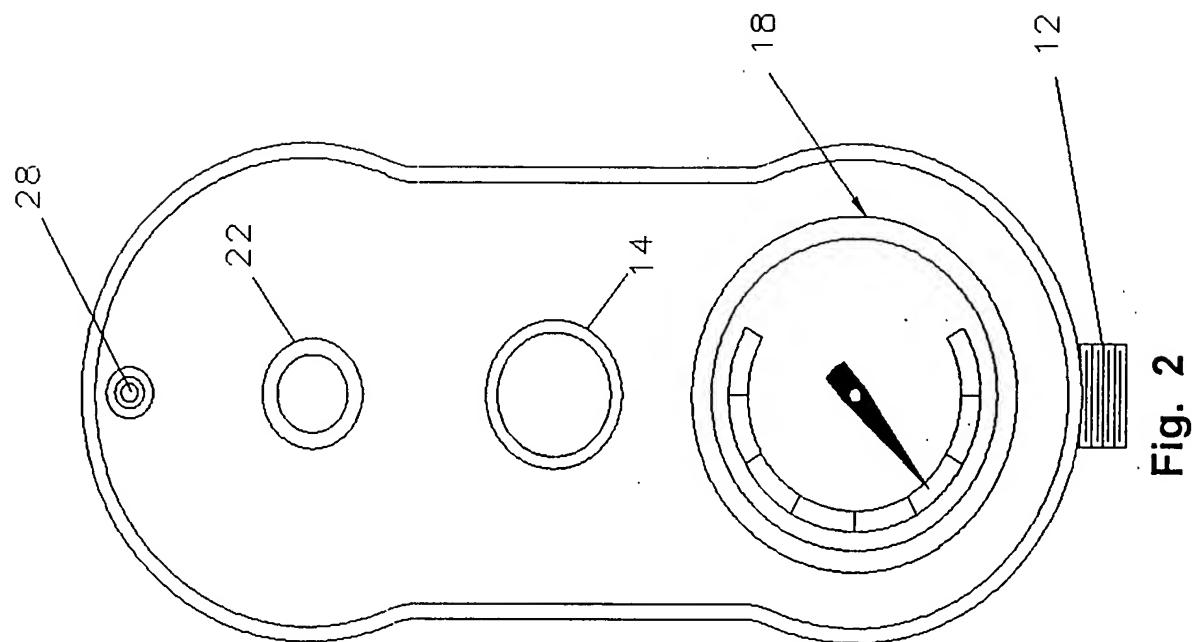


Fig. 2



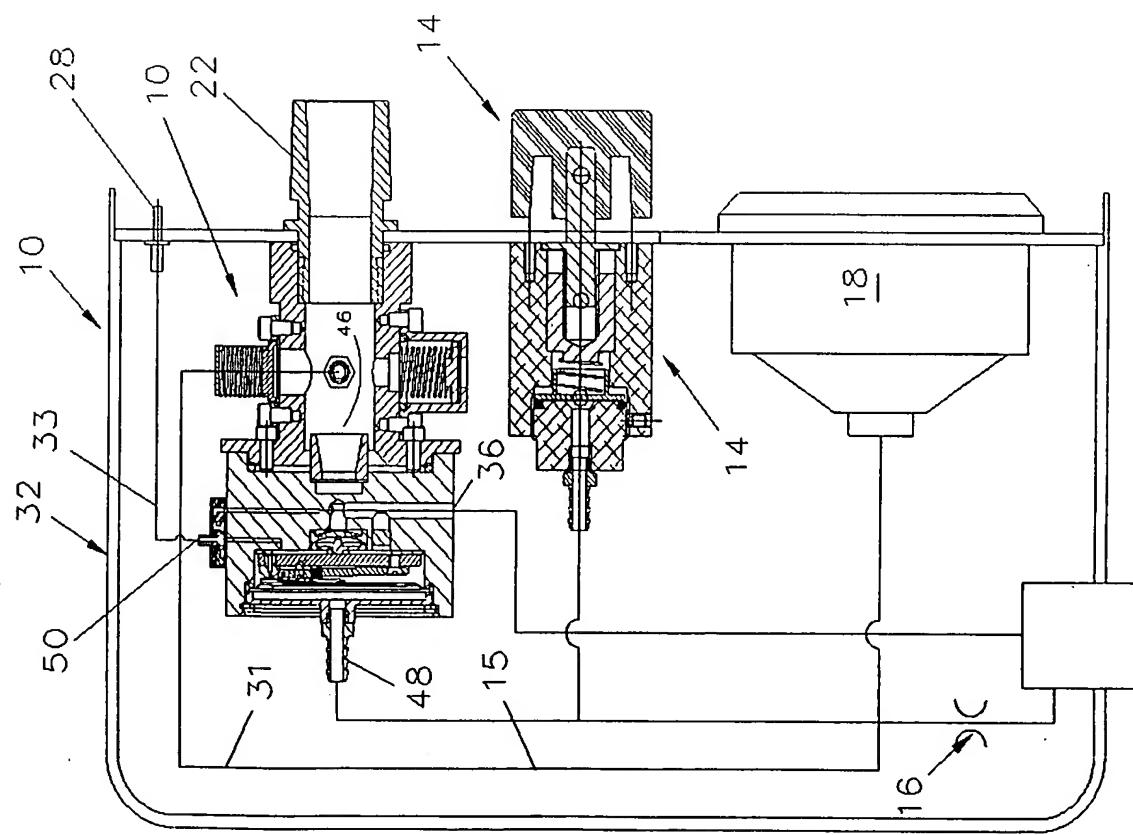


Fig. 3


U.S. Patent & Trademark Office

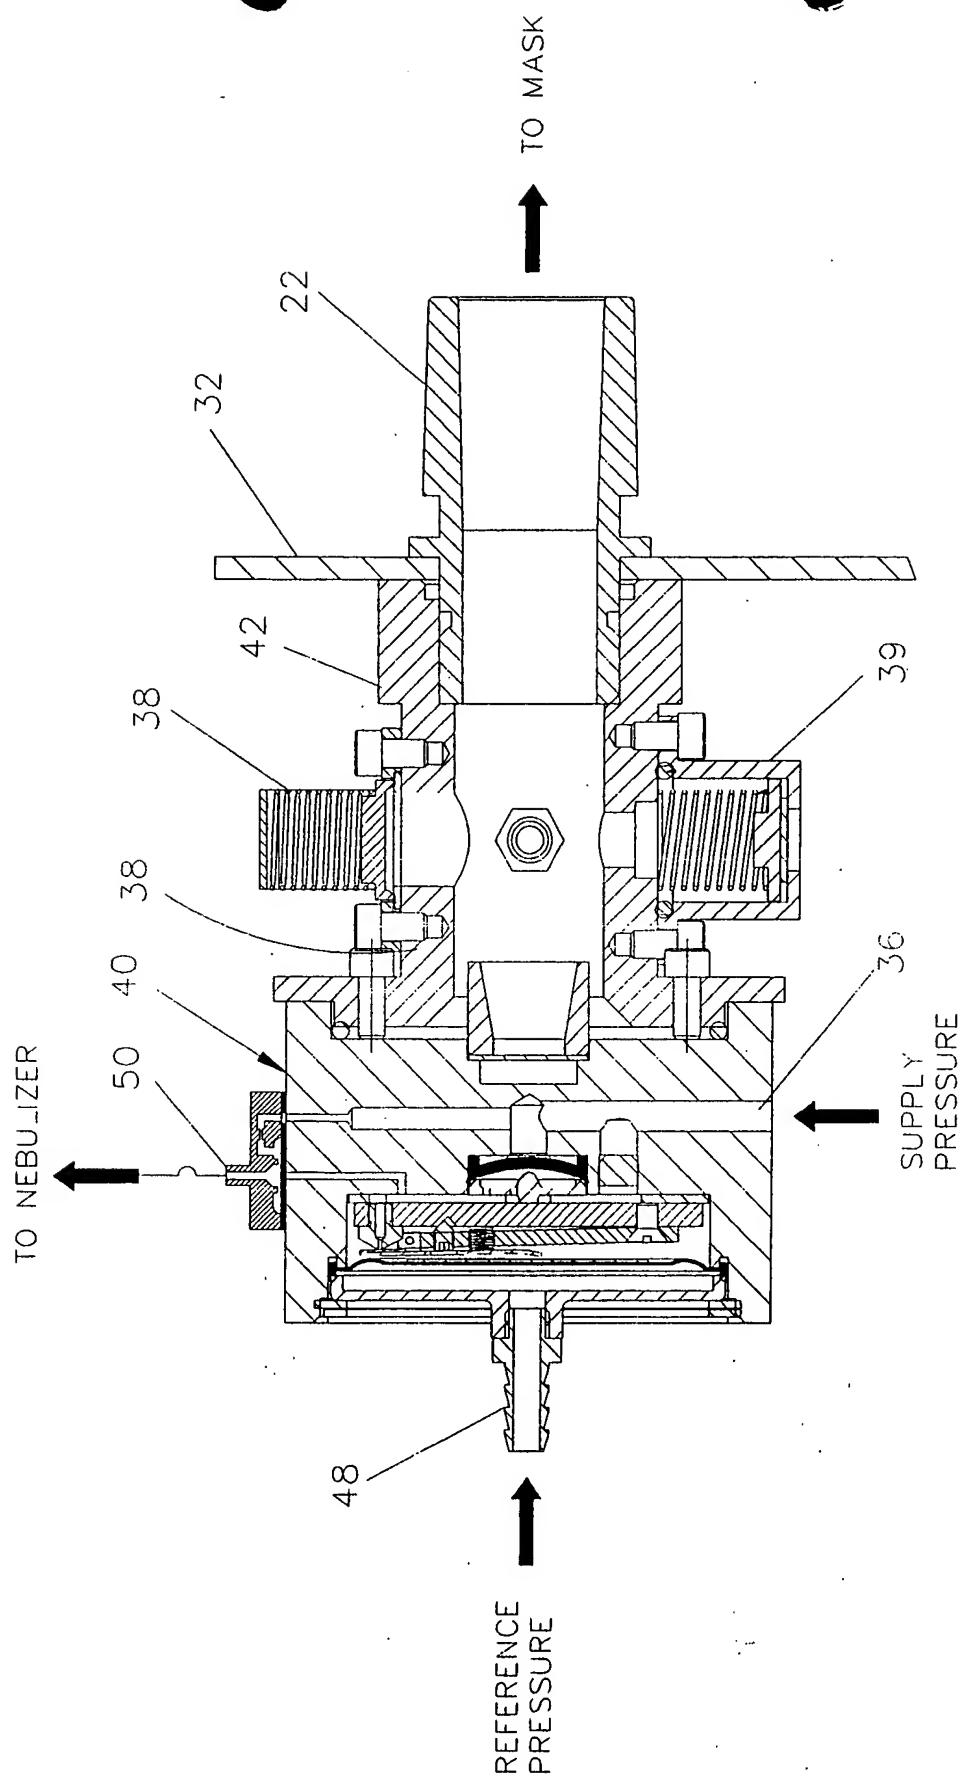

**Fig. 4**

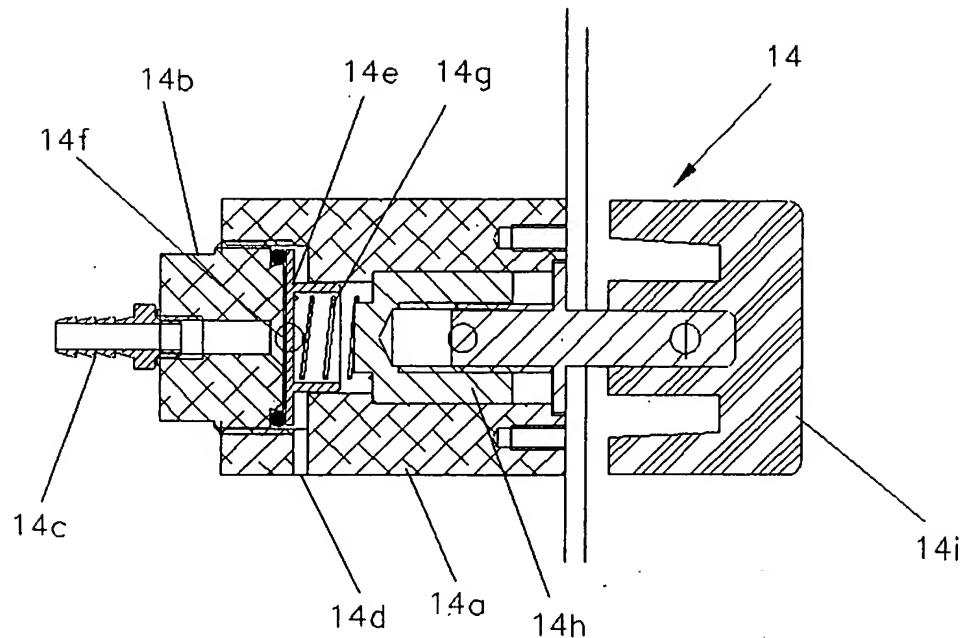


**Fig. 5**

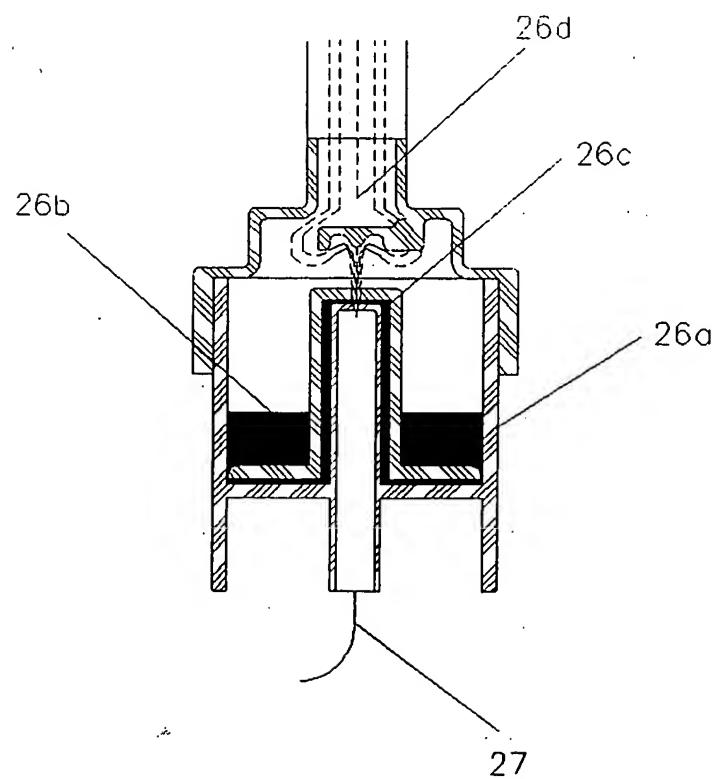

**Fig. 6**


2020年3月20日

1000000000000000

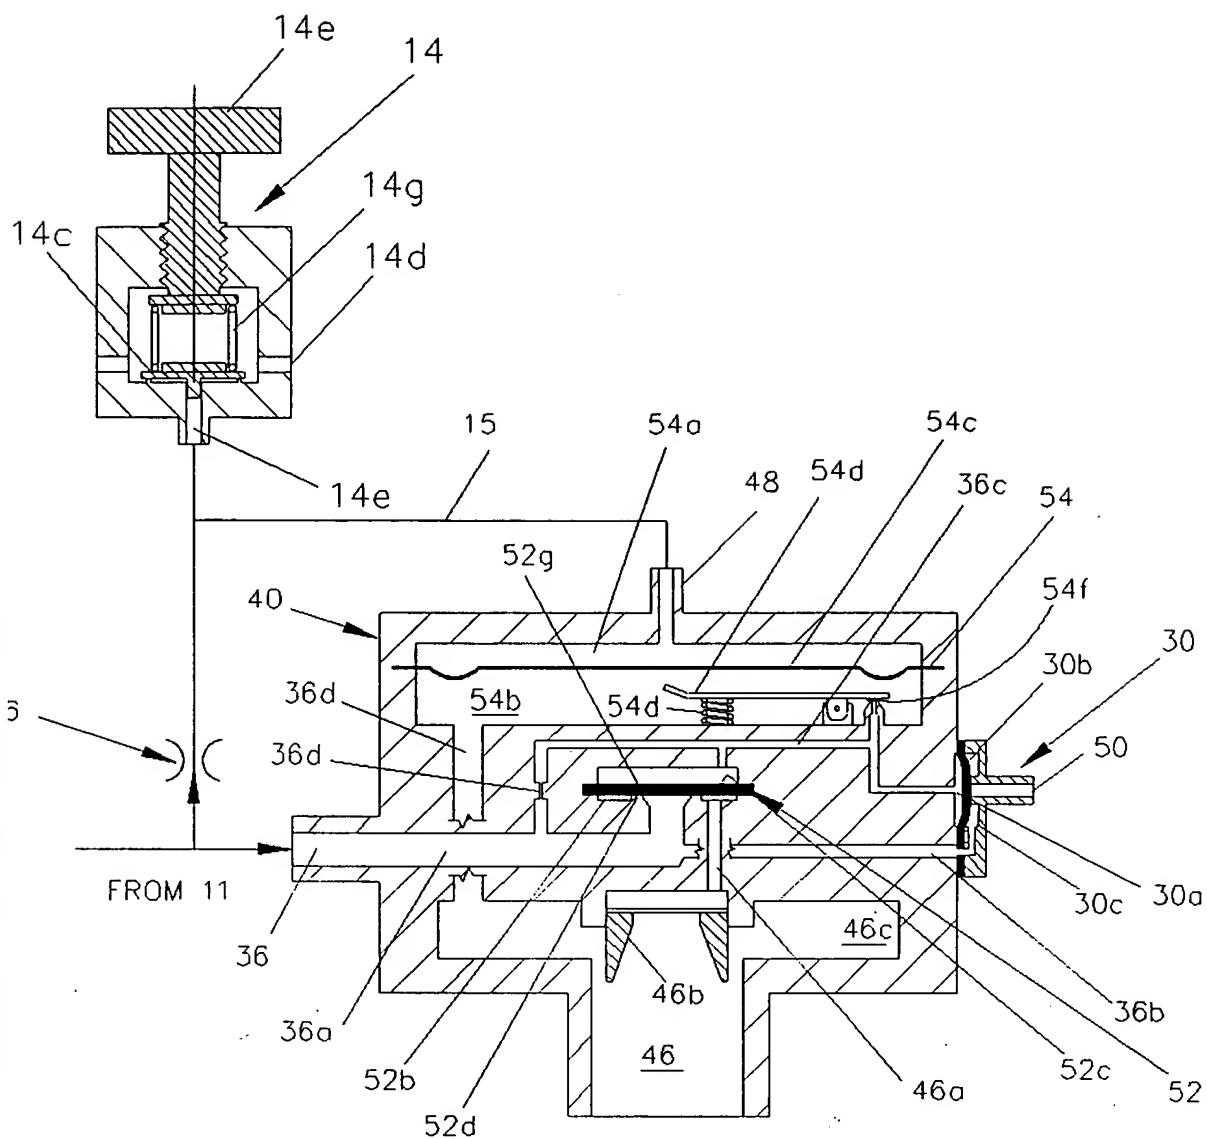


**Fig. 7 (EXHALATION)**

10000000000000000000000000000000

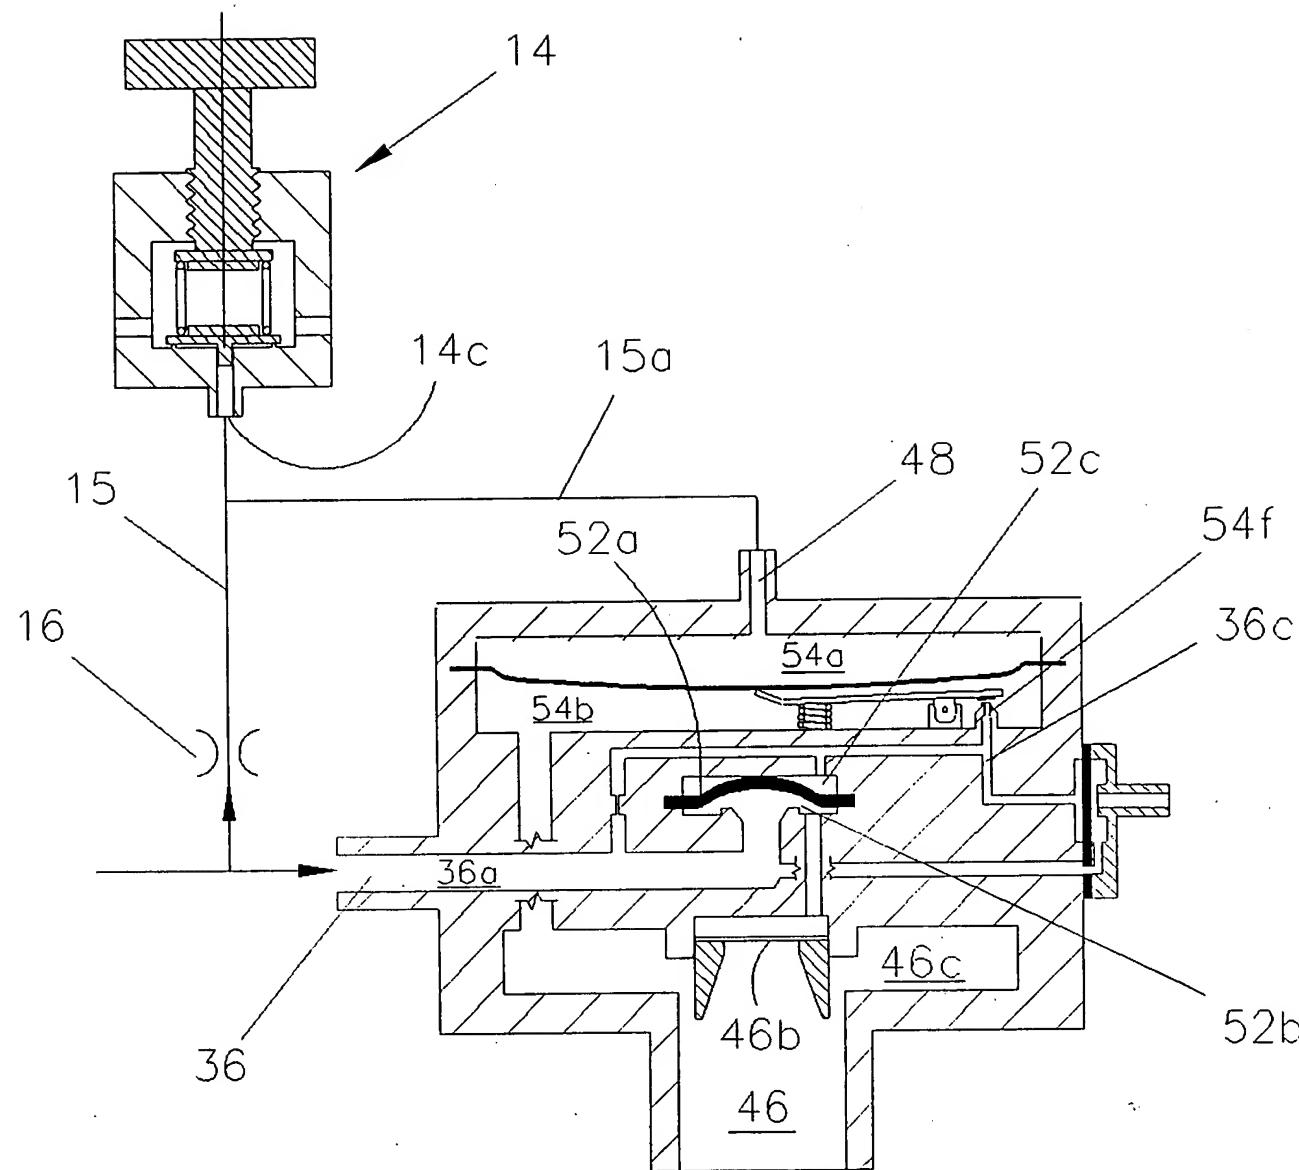


**Fig. 8 (INHALATION)**

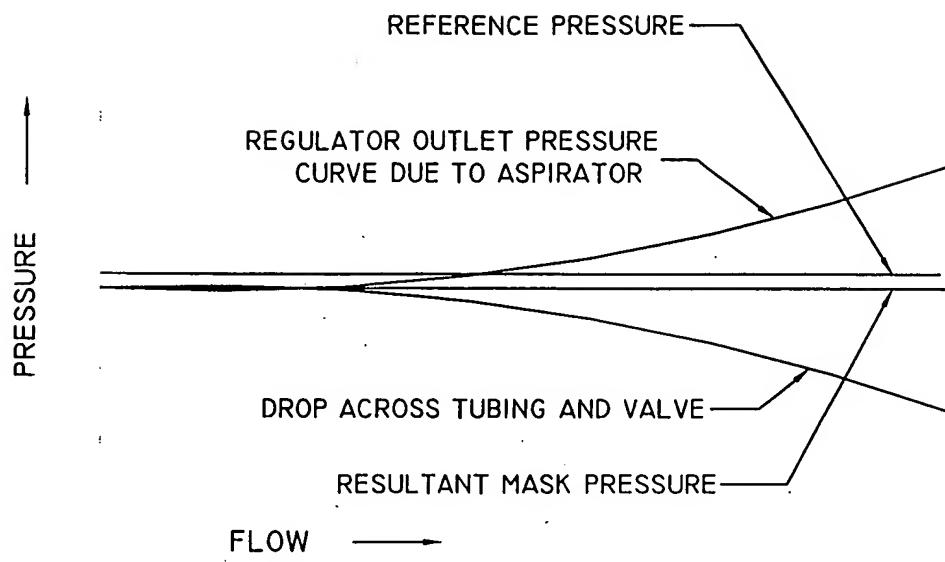


**Fig. 9**

10020544 312901

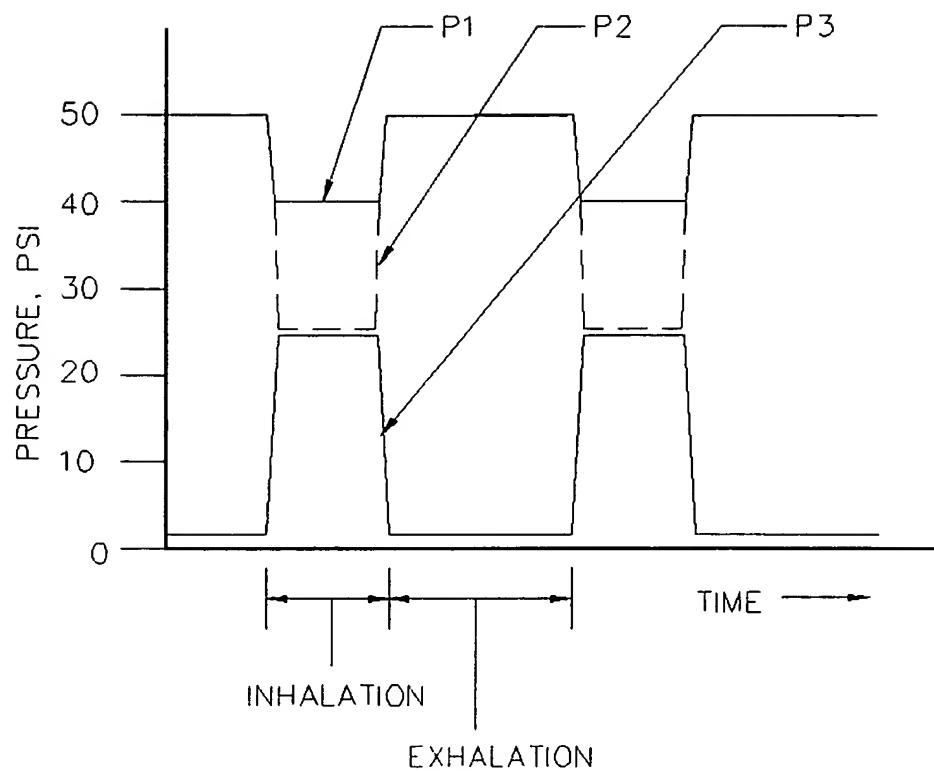


**Fig. 12**

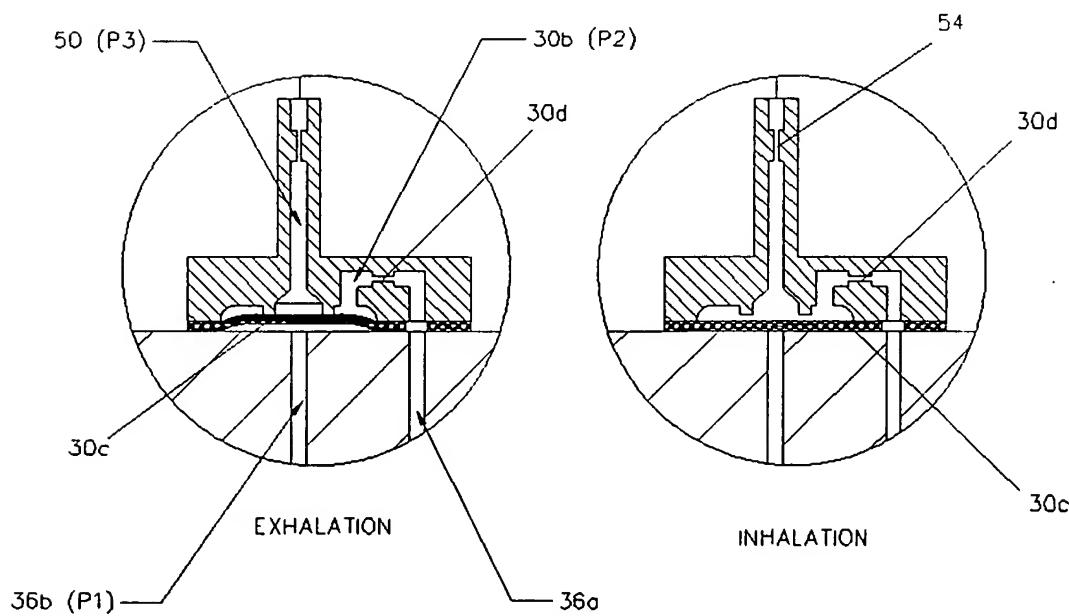


**Fig. 10**

**Fig. 11**

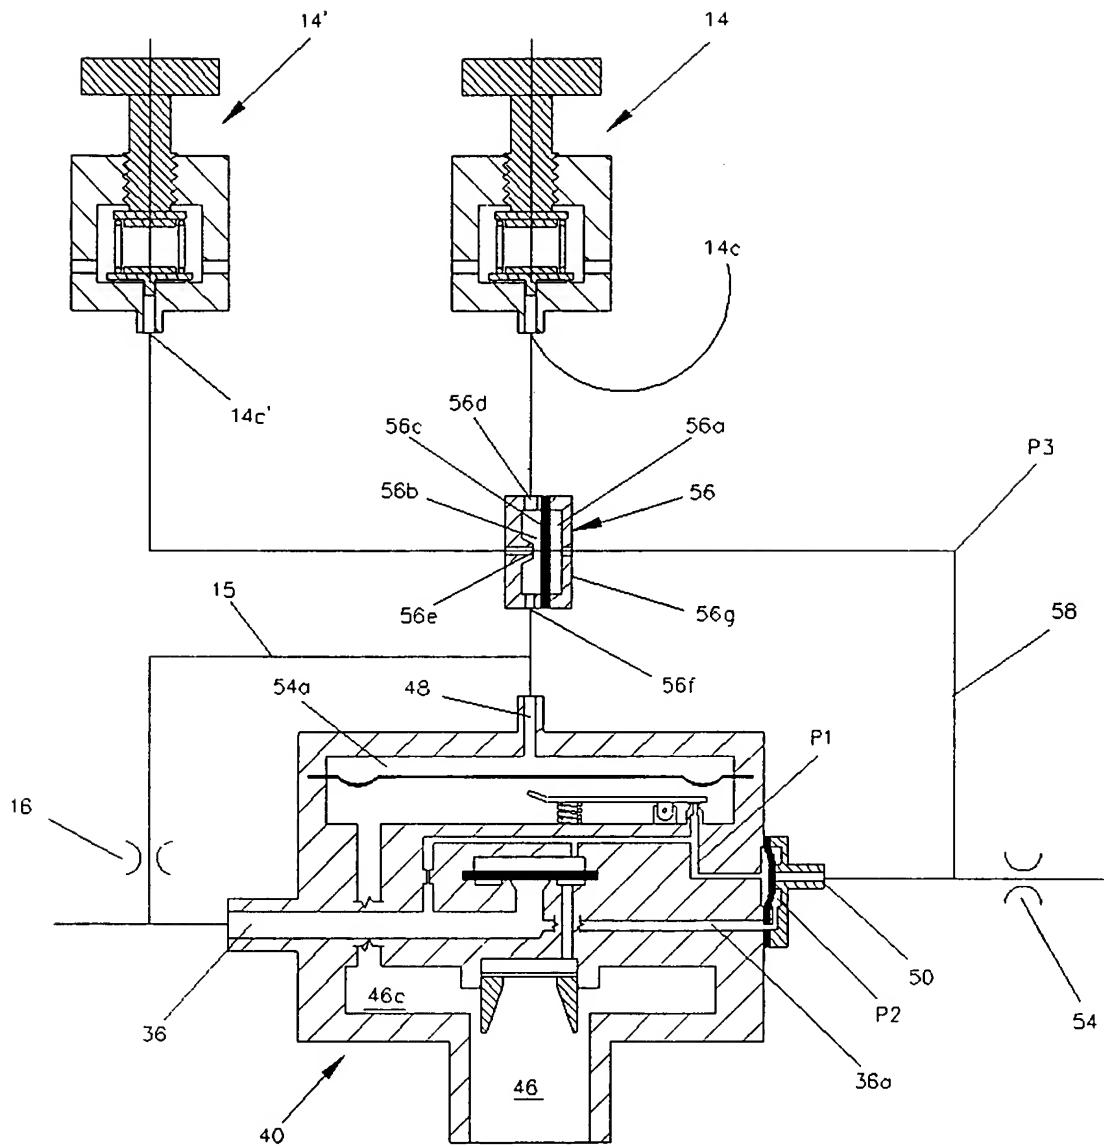

**Fig. 13 - EXHALATION**

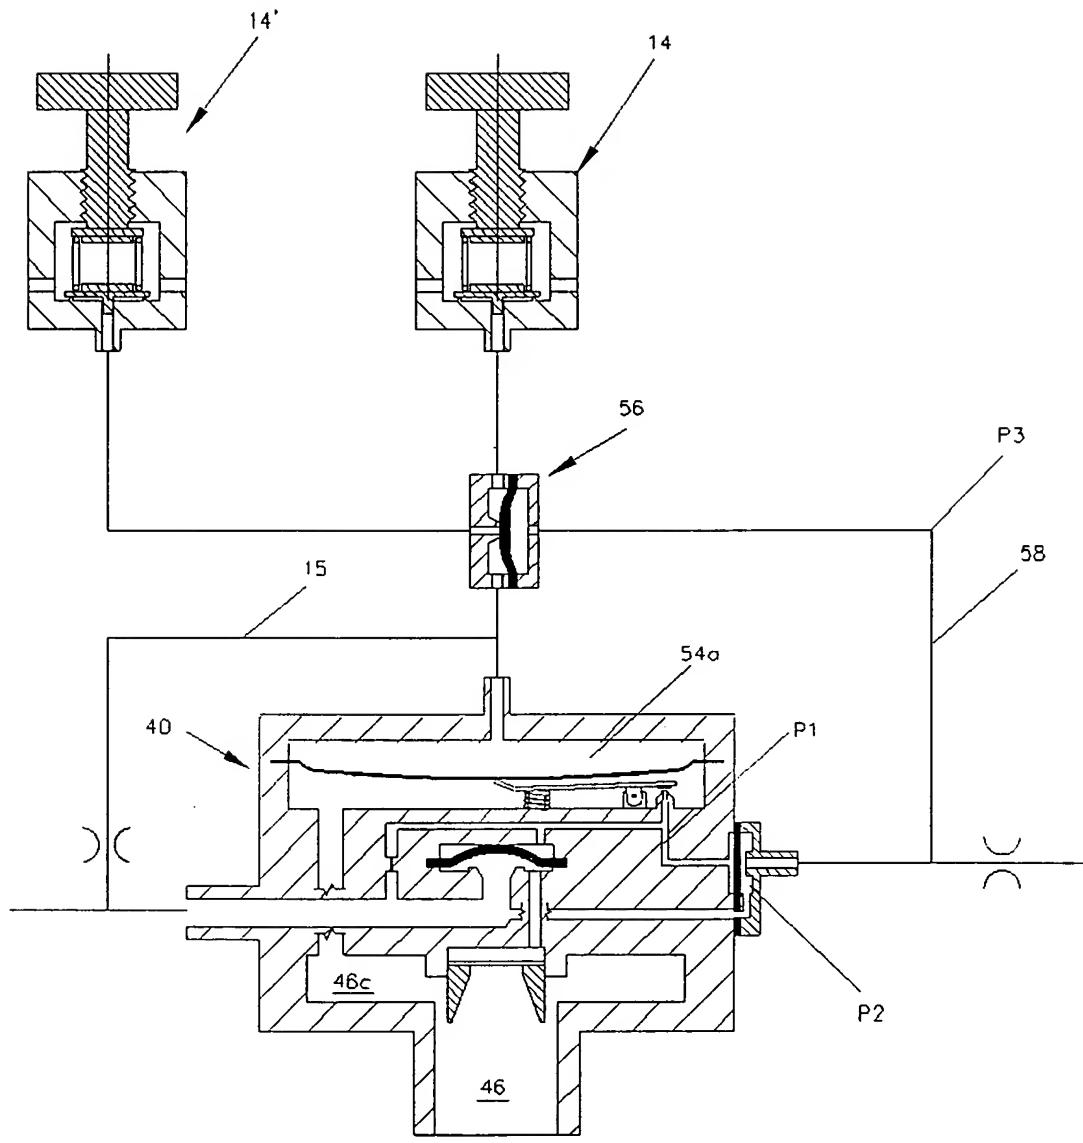

**Fig. 14 - INHALATION**

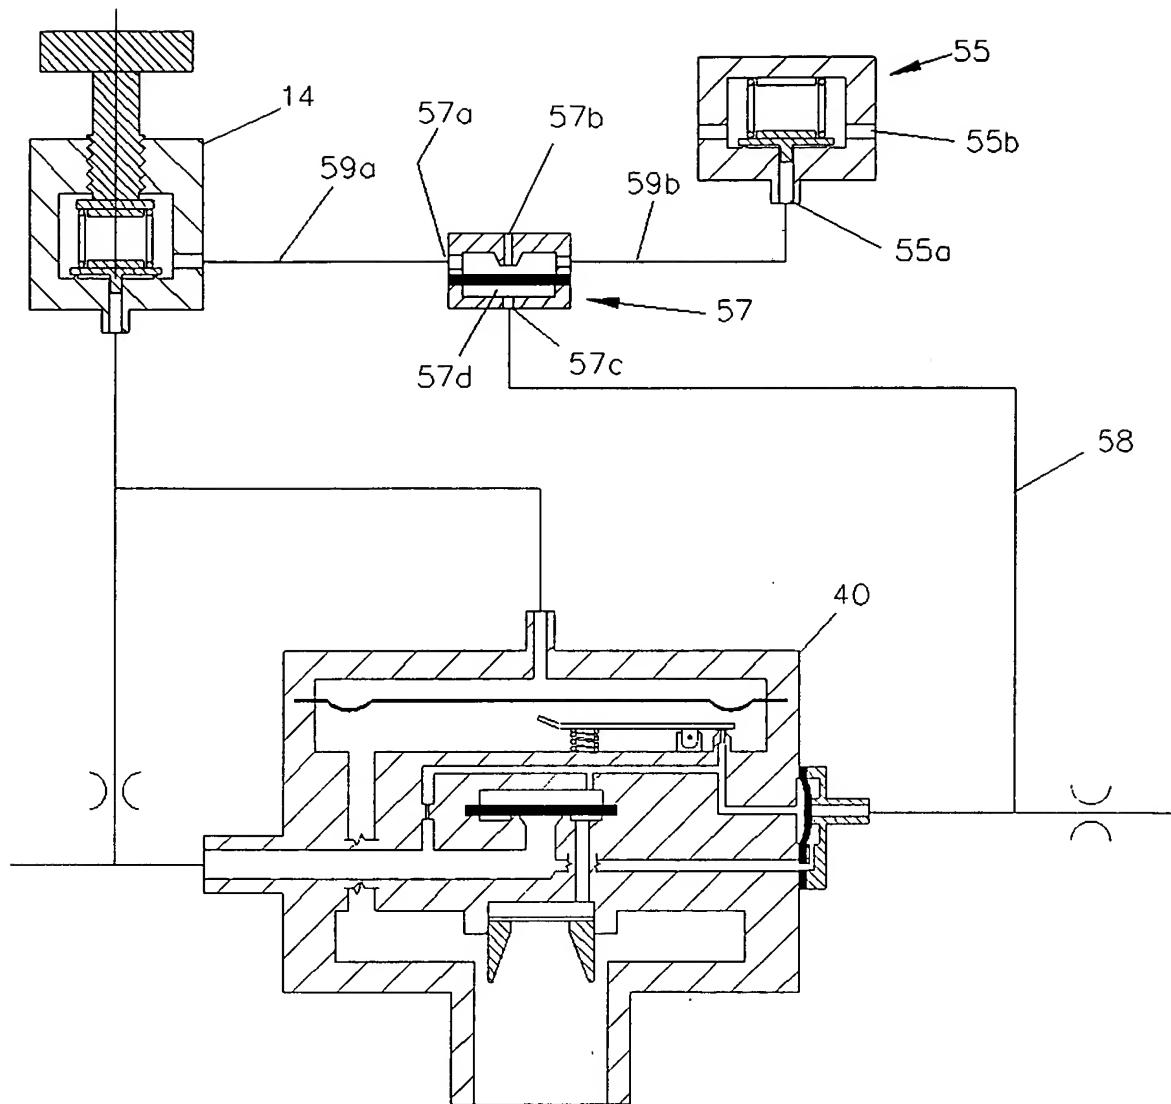


Fig. 15



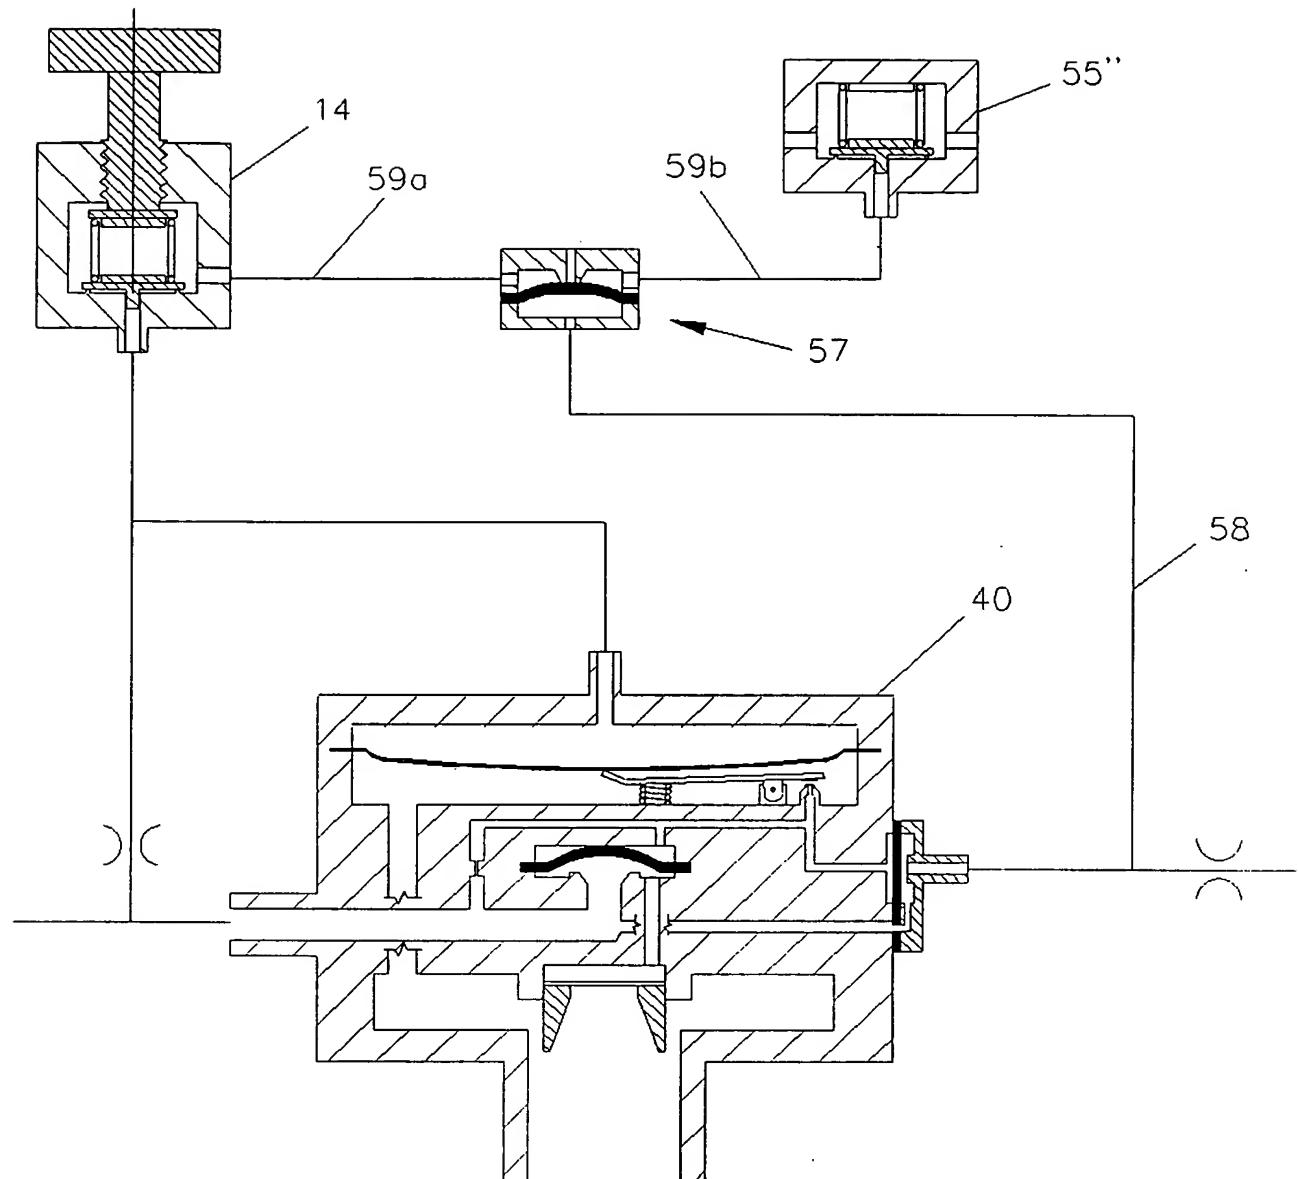


Fig. 16

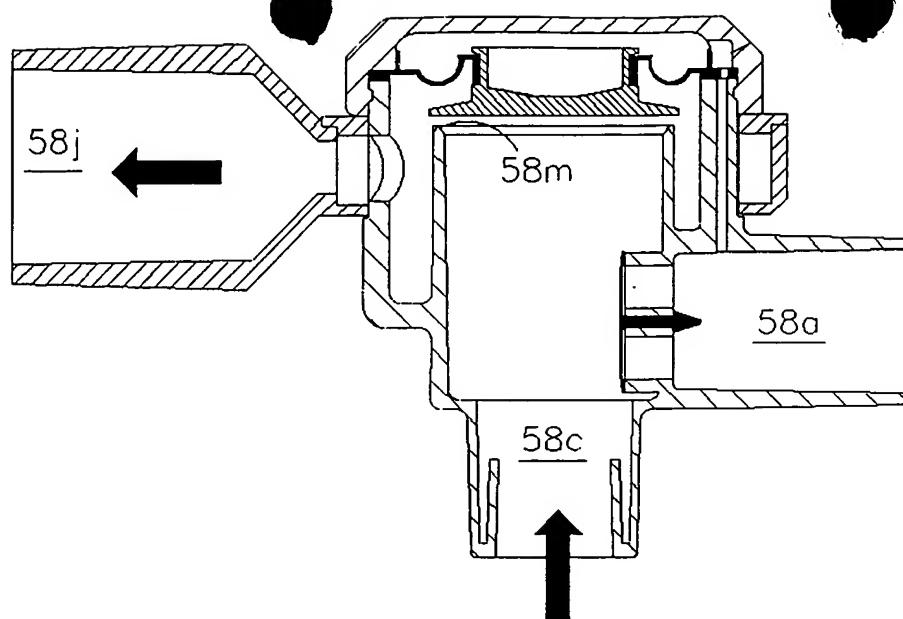

**Fig. 17 EXHALATION**

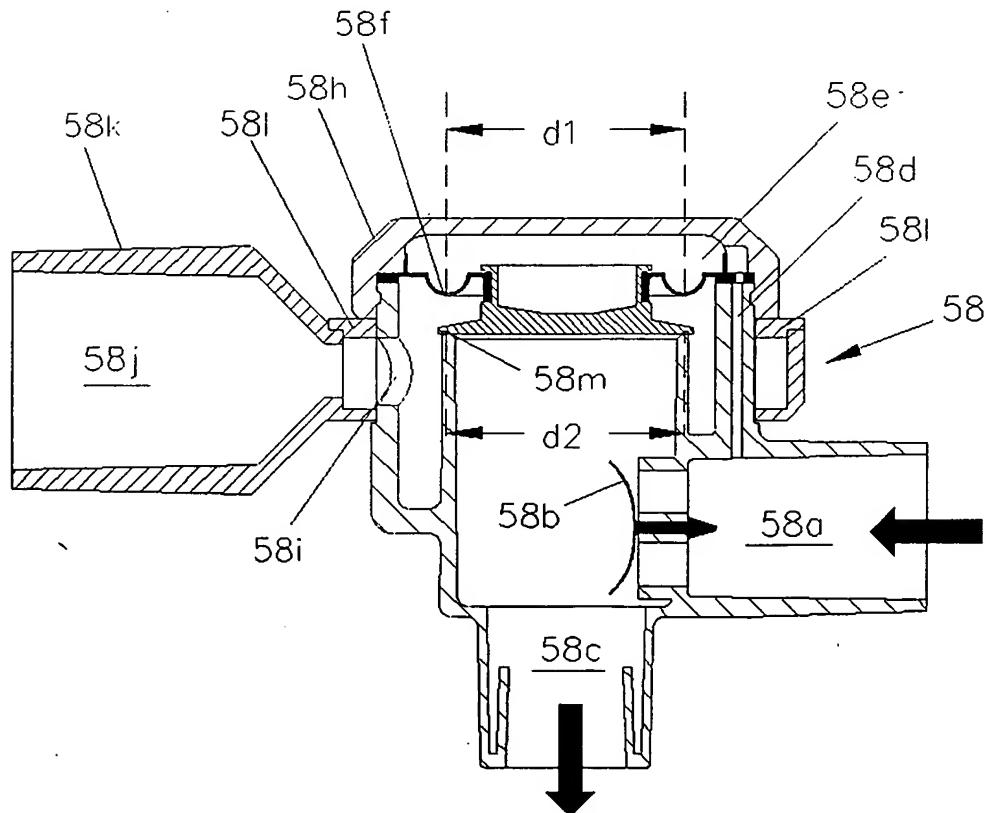

**FIG. 18 INHALATION**

2020020514471126017

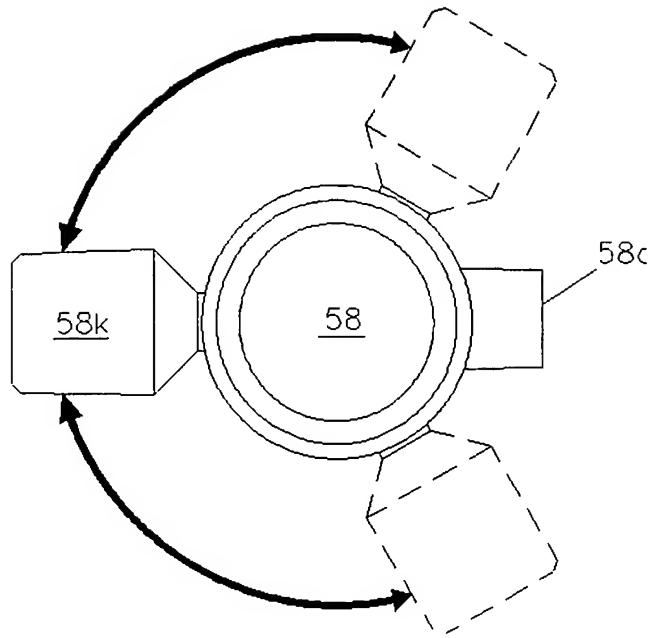


Fig. 19